

Myeloid Panel

The **oncoReveal™ Myeloid Panel** is a robust NGS assay that interrogates 58 genes of interest* most relevant to myeloid cancers. The panel uses proprietary Stem-Loop Inhibition-Mediated amplification (SLIMamp®) technology, a tiled amplicon-based library prep chemistry for efficient single-tube target enrichment.

oncoReveal™ Myeloid Panel (58 genes)

ABL1	BRAF	CEBPA	ETV6	HRAS	KDM6A	NPM1	PTEN	SMC1A	TP53
ANKRD26	CALR	CSF3R	EZH2	IDH1	KIT	NRAS	PTPN11	SMC3	U2AF1
ASXL1	CBL	CUX1	FLT3	IDH2	KMT2A	PDGFRA	RAD21	SRSF2	WT1
ATRX	CBLB	DDX41	GATA1	IKZF1	KRAS	PHF6	RUNX1	STAG1	ZRSR2
BCOR	CBLC	DNMT3A	GATA2	JAK2	MPL	PIGA	SETBP1	STAG2	
BCORL1	CDKN2A	ETNK1	GNAS	JAK3	NF1	PPM1D	SF3B1	TET2	

Genes marked in green indicate full CDS coverage

Simple NGS library prep workflow

Maintain control of samples and results with single-tube, tiled amplification that can be performed in-house by any NGS lab


Sensitive and robust chemistry

Achieve variant detection as low as 1% VAF[†] without UID[‡] even with limited DNA input or poor sample quality

Reduced fully-loaded lab costs

Improve lab efficiency and reduce “no calls”, repeat testing, and difficult interpretation decisions

Simple, one-day workflow

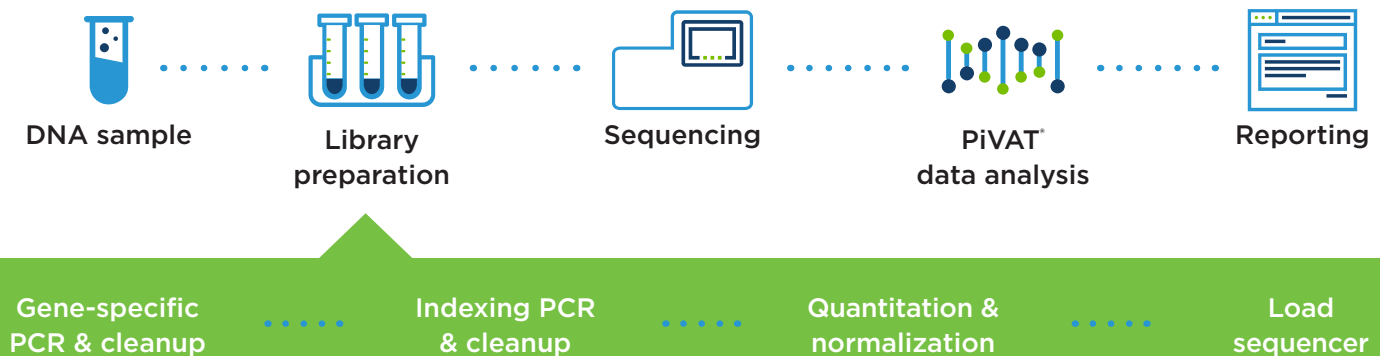

* Content is based on data from ongoing clinical trials along with sources that include the College of American Pathologists (CAP), the Association for Molecular Pathology (AMP), the National Comprehensive Cancer Network (NCCN), and the Catalog of Somatic Mutations in Cancer (COSMIC) database.

[†]UID, unique ID; also known as unique molecular ID (UMI); [‡]VAF, variant allele frequency
For Research Use Only. Not for use in diagnostic procedures.

Panel specifications*

Enrichment chemistry	Multiplex PCR using tiled amplicons
Number of pools	1 pool
Number of genes/amplicons	58/766
Number of targets	Full CDS coverage of 18 genes, hotspots in 40 additional genes, FLT3 ITDs; 107.9kb total size
Variant types	SNVs, indels, ITD (internal tandem duplicates)
Average amplicon size	217bp
Recommended DNA input range	20ng to 60ng (20ng recommended)
Sample types	DNA from whole blood, PBMCs
Mapping rate	99.6% ± 0.2%
% on-target aligned reads	92.0% ± 5.3%
Coverage uniformity (% targets with >0.2X mean coverage)	96.8% ± 1.0%
Recommended Reads Per Sample	~4 million paired-end reads
Total assay time (from DNA to sequencer)	<8 hours

* Mapping rate, percentage of on-target aligned reads, and coverage uniformity metrics are based on internal testing performed using reference standard materials

Ordering information

Select the panel AND one of the index kit options listed below.

Panel	Part number
oncoReveal™ Myeloid Panel (24 reactions)	HDA-MY-1001-24

Pillar Index Kit options	Reactions	Part number
Pillar Custom Index Primers Kit A	32 Combinations, 96 reactions	IDX-PI-1001-96
Pillar Custom Index Primers Kit D	96 Combinations, 192 reactions	IDX-PI-1004-192

TO ORDER OR LEARN MORE:
pillarbiosci.com

For research use only. Not for use in diagnostic procedures.

© 2022 Pillar Biosciences. Pillar®, SLIMamp®, PIVAT® and oncoReveal™ are trademarks of Pillar Biosciences, Inc. Current as of 10.15.2023 | MK-0007-4 v1.1

PILLAR
 BIOSCIENCES

Pillar Biosciences, Inc.
 9 Strathmore Rd
 Natick, MA 01760
 (800) 514-9307
info@pillarbiosci.com